

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
19 July 2001 (19.07.2001)

PCT

(10) International Publication Number
WO 01/50941 A2

- (51) International Patent Classification⁷: A61B
- (21) International Application Number: PCT/IL01/00020
- (22) International Filing Date: 10 January 2001 (10.01.2001)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
134017 13 January 2000 (13.01.2000) IL
- (71) Applicant and
(72) Inventor: REFAEL, Moshe [IL/IL]; 83 Eitanim str.,
36001 Nofit (IL).
- (74) Agent: MILLER-SIERADZKI, ADVOCATES &
PATENT ATTORNEYS; P.O.B. 6145, 31061 Haifa (IL).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU,
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CR, CU, CZ,

DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR,
HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR,
LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ,
NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM,
TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.

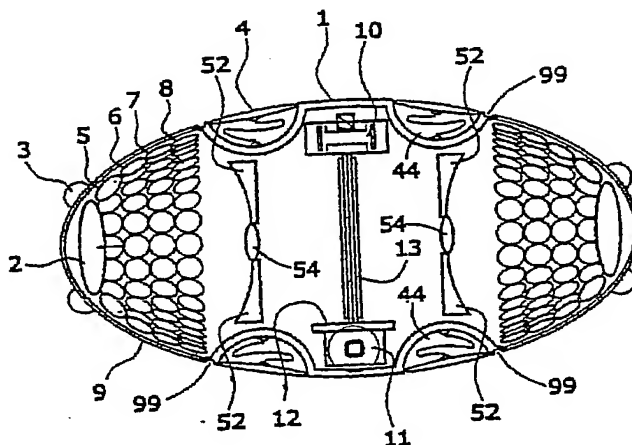
(84) Designated States (regional): ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian
patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European
patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE,
IT, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BJ, CF,
CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

Published:

— without international search report and to be republished
upon receipt of that report

For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.

(54) Title: ENCAPSULATED MEDICAL IMAGING DEVICE AND METHOD



WO 01/50941 A2

(57) Abstract: An encapsulated medical imaging system is disclosed, comprising: a capsule of swallowable proportion comprising at least one optical setup of a number of optical setups comprising an array of microlenses distributed in axial symmetry on at least a portion of the capsule so that the array of microlenses is capable of receiving light reflected from object located in at least a sector outside the capsule; corresponding optical array comprising an array of light sensitive cells optically communicating with said optical setup through focusing means, such that the image of the object is focused on the array of light sensitive cells; electronic circuitry adapted to sample image data obtained by the optical array by scanning the image and converting the image data to digital data; illuminating means for illuminating a sector in front the optical setup, outside the capsule; transmitting means communicating with said electronic circuitry, adapted to receive image digital data and transmit it to an external receiver; receiving means for receiving data transmitted from said capsule; image processing means for processing the data received by the receiving means and; and display means for displaying an image.

ENCAPSULATED MEDICAL IMAGING DEVICE AND METHOD

FIELD OF THE INVENTION

The present invention relates to medical imaging. More particularly it
5 relates to an encapsulated medical imaging device and method for imaging
gastro intestinal tract in patients, using scanning technologies.

BACKGROUND OF THE INVENTION

The gastrointestinal tract in adult humans is about 7-9 meters in total.
10 Presently, of these 7-9 meters only as much as about 1.2 meters, extending
from the ends of the gastrointestinal (GI) tract inwardly, may be imaged in
commonly practiced medical imaging techniques (colonoscopy). Usually such
imaging techniques involve inserting a tubular optical device (such as fiber
optics) into the upper digestive system through the mouth (gastroscopy) or
15 into the colon through the anus (colonoscopy) and advancing it along the
gastrointestinal tract to inspect it and detect the presence of pathologies.

It may take years for a colon polyp to grow and turn malignant. In the
absence of neurological warning system to indicate the occurrence of
malignancies in their early stages it is often that the diagnosis of
20 gastrointestinal malignancies is too late to be cured. Problems in the GI tract
are ever too often detected only when they appear in great gravity and even
then detection is made possible through the discovery of secondary
indications (such as fecal occult blood occurrence). Early detection can be a
major factor in improving the patient's chances of survival.

25 Some of the commonly occurring GI diseases include GI internal
bleeding, inflammations of the GI tract, polyps, tapering of the GI tract,
intestinal perforation, arteriovenous malformation. Internal bleeding may be

caused by ulcer or varicose veins. These diseases cannot be detected in X-ray imaging or other non-invasive imaging methods until they evolve to traumatic proportion, yet even when diagnosed it is difficult to point out their exact location if that happens to fall beyond the inspectable range.

5 GI tract cancers are considered major factor in older adults fatalities. Gastrointestinal malignancies are considered to be the 2nd highest factor in male fatalities, and 3rd highest factor in female fatalities. GI diseases may be classified with reference to their location in the GI tract and the distribution of these diseases was found to be as follows: 30 per cent occurring in the
10 esophagus, stomach and duodenum, 10 per cent occurring in the small intestine and some 60 percent occurring in the large intestine.

The inability to image the small intestine may bring about the need to perform investigative abdomen incision, sometimes just for ruling out a vague suspicion of malignancy.

15 Although some 80 per cent of the GI diseases may supposedly be detected by colonoscopy or gastroscopy, sometimes these invasive techniques may be considered undesired. These techniques are relatively costly, requiring the presence of a several member medical team throughout the procedure. Furthermore it is statistically shown that about one in 2000
20 patients is prone to perforation of the GI tract caused by a sharp object (the imaging tool) during the performance of the procedure. Such an incident immediately requires surgical intervention.

US 5,604,531 (Iddan et al.) entitled IN-VIVO VIDEO CAMERA SYSTEM, filed in 1995, and incorporated herein by reference, discloses an in-
25 vivo video camera system and an autonomous video endoscope. The system includes a swallable capsule, a transmitter and a reception system. The swallable capsule includes a camera system and an optical system for imaging an area of interest onto the camera system. The transmitter transmits the output of the video camera system and the reception system receives the
30 transmitted video output.

US 4,278,077 (Mitzumoto) entitled MEDICAL CAMERA SYSTEM, filed in 1979, and incorporated herein by reference, discloses a capsule-shaped miniature camera comprising at least one permanent magnet, an induction coil, a lamp serially connected to the induction coil and a shutter device. The induction coil induces an electromotive force when a magnetic field generated by electromagnets outside the camera acts on it. The electromotive force turns on the lamp and drives the shutter device.

The video camera system of the '531 patent (Iddan) employs analog video and analog transmission. It is evident that it provides an image focused at a predetermined fixed distance from the optical lens and consequently, due to the poor lighting conditions within the GI tract, blurred image of objects falling outside or falling short of the focal range. As the GI tract is composed of parts of different diameters (the esophagus, stomach, small and large intestines) it is anticipated that substantial information will be omitted or severely degraded in the image obtained by Iddan's system. Furthermore the inside walls of the GI tract are also present "hilly" topography, and therefore pose difficulties to the imaging abilities of that system.

It is noted that these prior art optical imaging devices are limited in their field of view as they include a single optical system and are therefore limited to one directional view. For irregular surfaces as exist in the GI tract this may result in many hidden areas that the imager will not view properly. Furthermore the possibility of the capsule flopping over or turning around is real and may hamper with the proper functionality of the device.

BRIEF DESCRIPTION OF THE INVENTION

It is therefore thus provided, in accordance with a preferred embodiment of the present invention, an encapsulated medical imaging system comprising:

a capsule of swallowable proportion comprising:

at least one optical setup of a number of optical setups comprising an array of microlenses distributed in axial symmetry on at least a portion of the capsule so that the array of microlenses is capable of receiving light reflected from object located in at least a sector outside the capsule;

corresponding optical array comprising an array of light sensitive cells optically communicating with said optical setup through focusing means, such that the image of the object is focused on the array of light sensitive cells;

electronic circuitry adapted to sample image data obtained by the optical array by scanning the image and converting the image data to digital data;

illuminating means for illuminating a sector in front the optical setup, outside the capsule;

transmitting means communicating with said electronic circuitry, adapted to receive image digital data and transmit it to an external receiver;

receiving means for receiving data transmitted from said capsule;

image processing means for processing the data received by the receiving means and; and

display means for displaying an image.

Furthermore, in accordance with another preferred embodiment of the present invention, the number of the optical setups comprises two optical setups, arranged in opposite sides of the capsule, so as to allow counter-directional viewing.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is provided with at least one lens of a number of lenses for central view and wherein the array of microlenses is arranged in a coronal arrangement with respect to the lens, so as to provide peripheral
5 view.

Furthermore, in accordance with another preferred embodiment of the present invention, the number of lenses comprises two lenses.

Furthermore, in accordance with another preferred embodiment of the present invention, the microlens array comprises a plurality of microlenses
10 having different foci distributed in a known distribution, and wherein the processing means is adapted to identify and distinguish focused image data from unfocused one, disregard the unfocused data and acquire image made of focused data only.

Furthermore, in accordance with another preferred embodiment of the present invention, the illumination means comprises light emitting diodes.
15

Furthermore, in accordance with another preferred embodiment of the present invention, the light emitting diodes illuminate light in different frequency ranges.

Furthermore, in accordance with another preferred embodiment of the present invention, the light emitting diodes emit red, green or blue light.
20

Furthermore, in accordance with another preferred embodiment of the present invention, the light emitting diodes are operated so as to sequentially illuminate red green and blue light.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is about 12-20 mm in length and about 5-7 mm in diameter.
25

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule housing is made from a biocompatible material.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule housing is made from a dissolvable material.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule housing is made from a dissolvable material
5 that is durable enough so that it may pass an entire GI tract without disintegrating during the estimated period of time it would normally take for the capsule to pass through.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is internally powered.

10 Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is externally powered.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is inductively powered.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is further provided with supporting means for
15 supporting the capsule and preventing its turning over or around.

Furthermore, in accordance with another preferred embodiment of the present invention, said supporting means comprise extractable surfaces.

Furthermore, in accordance with another preferred embodiment of the present invention, the extractable surfaces are supported by arms.
20

Furthermore, in accordance with another preferred embodiment of the present invention, said arms are resilient.

Furthermore, in accordance with another preferred embodiment of the present invention, said arms are mechanically foldable.

Furthermore, in accordance with another preferred embodiment of the present invention, the arms are adapted to be housed in cavities provided in the housing of the capsule.

Furthermore, in accordance with another preferred embodiment of the present invention, the cavities are adapted to hold samples obtained by the arms.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is further provided with a medical parameter sensor.

Furthermore, in accordance with another preferred embodiment of the present invention, the sensor comprises a temperature sensor or a pressure sensor.

Furthermore, in accordance with another preferred embodiment of the present invention, the capsule is further provided with wiping means for wiping dirt off the optical setup.

Furthermore, in accordance with another preferred embodiment of the present invention, the wiping means comprises a wiping arm.

Finally, in accordance with another preferred embodiment of the present invention, there is provided an encapsulated medical imaging system comprising:

a capsule of swallowable proportion comprising:

at least one optical setup of a number of optical setups comprising an array of multi-focal lenses distributed in axial symmetry on at least a portion of the capsule so that the array of multi-focal lenses is capable of receiving light reflected from object located in at least a sector outside the capsule;

- corresponding optical array comprising an array of light sensitive cells optically communicating with said optical setup through focusing means, such that the image of the object is focused on the array of light sensitive cells;
- 5 electronic circuitry adapted to sample image data obtained by the optical array by scanning the image and converting the image data to digital data;
- illuminating means for illuminating a sector in front the optical setup, outside the capsule;
- 10 transmitting means communicating with said electronic circuitry, adapted to receive image digital data and transmit it to an external receiver;
- receiving means for receiving data transmitted from said capsule;
- image processing means for processing the data received by the receiving means and; and
- 15 display means for displaying an image.

BRIEF DESCRIPTION OF THE FIGURES

In order to better understand the present invention, and appreciate its practical applications, the following Figures are provided and referenced hereafter. It should be noted that the Figures are given as examples only and in no way limit the scope of the invention as defined in the appending Claims. Like components are denoted by like reference numerals.

Figure 1a illustrates a patient's GI tract with an encapsulated medical imaging device in accordance with the present invention traveling through it.

Figure 1b illustrates a general view of an encapsulated medical imaging device in accordance with a preferred embodiment of the present invention.

5 Figure 2a illustrates the encapsulated medical imaging device of the present invention provided with arms, shown in semi-retracted state as it travels through a small intestine.

Figure 2b depicts the encapsulated medical imaging device of Fig. 2a with its arms fully deployed as it travels through a large intestine.

10 Figure 3a is a see-through view of a preferred embodiment of the encapsulated medical imaging device of the present invention.

Figure 3b depicts the optical scheme of the device of Fig. 3a.

Figure 4a illustrates a single stretched row of the microlens array of the device of Fig. 3a.

15 Figure 4b, illustrates fields of view of an encapsulated medical imaging device in accordance to the present invention as it travels through an intestine.

Figures 5a, 5b and 5c illustrate a display monitor communicating with a receiving unit of an encapsulated medical imaging device of the present invention incorporated in a vest worn by a patient.

20 Figure 6 illustrates a way to calculate the correct position of a suspected pathology detected by the encapsulated medical imaging device of the present invention.

Figure 7 illustrates an optional schematic configuration of the electronic system of an encapsulated medical imaging device in accordance with a preferred embodiment of the present invention.

25

DETAILED DESCRIPTION OF THE INVENTION AND FIGURES

A main aspect of the present invention is the provision of a multi-focal hemispherical-like array, capable of capturing focused images of various portions of the inspected objects located at different distances from the capsule.

Another main aspect of the present invention is the provision of optical array and the performance of scanning of the object rather than simply taking pictures frame-by-frame. The resolution of the image is determined by the number of pixels, which corresponds to the number of photosensors of a optical array utilized in the present invention. Scanning allows greater resolution to be attained in comparison with video imaging (as suggested in Iddan's '531 patent), obtaining segment-by-segment image of the viewed object.

The structure and mode of operation of the encapsulated medical imaging device of the present invention is herein explained with reference to the accompanying Figures.

Reference is made to Figure 1a, illustrating a patient's GI tract with an encapsulated medical imaging device in accordance with the present invention traveling through it. Initially the patient 30 is made to swallow the capsule 1. Capsule 1, having dimensions suitable for it to be taken orally and swallowed, after having been swallowed, immediately starts transmitting image data. It is traveling through the patient's GI tract 35, the GI tract generally comprising the esophagus 38, stomach 32, small intestine 34 and large intestine 36. The capsule is shown located at the small intestine 34 of the patient, traveling through it and transmitting information as it travels through. Typical anticipated dimensions for the capsule would be approximately 12 - 20 mm in length and about 5-7 mm in diameter. The capsule housing is made of bio-compatible non-toxic matter.

The encapsulated medical imaging device generally includes optical system, illumination system, optical array for obtaining digital representation of the image obtained by the optical system, electronic circuitry, and transmitting

5
10
15
20
25
30
35
40
45
50
55
60
65
70
75
80
85
90
95
100
105
110
115
120
125
130
135
140
145
150
155
160
165
170
175
180
185
190
195
200
205
210
215
220
225
230
235
240
245
250
255
260
265
270
275
280
285
290
295
300
305
310
315
320
325
330
335
340
345
350
355
360
365
370
375
380
385
390
395
400
405
410
415
420
425
430
435
440
445
450
455
460
465
470
475
480
485
490
495
500
505
510
515
520
525
530
535
540
545
550
555
560
565
570
575
580
585
590
595
600
605
610
615
620
625
630
635
640
645
650
655
660
665
670
675
680
685
690
695
700
705
710
715
720
725
730
735
740
745
750
755
760
765
770
775
780
785
790
795
800
805
810
815
820
825
830
835
840
845
850
855
860
865
870
875
880
885
890
895
900
905
910
915
920
925
930
935
940
945
950
955
960
965
970
975
980
985
990
995
1000
1005
1010
1015
1020
1025
1030
1035
1040
1045
1050
1055
1060
1065
1070
1075
1080
1085
1090
1095
1100
1105
1110
1115
1120
1125
1130
1135
1140
1145
1150
1155
1160
1165
1170
1175
1180
1185
1190
1195
1200
1205
1210
1215
1220
1225
1230
1235
1240
1245
1250
1255
1260
1265
1270
1275
1280
1285
1290
1295
1300
1305
1310
1315
1320
1325
1330
1335
1340
1345
1350
1355
1360
1365
1370
1375
1380
1385
1390
1395
1400
1405
1410
1415
1420
1425
1430
1435
1440
1445
1450
1455
1460
1465
1470
1475
1480
1485
1490
1495
1500
1505
1510
1515
1520
1525
1530
1535
1540
1545
1550
1555
1560
1565
1570
1575
1580
1585
1590
1595
1600
1605
1610
1615
1620
1625
1630
1635
1640
1645
1650
1655
1660
1665
1670
1675
1680
1685
1690
1695
1700
1705
1710
1715
1720
1725
1730
1735
1740
1745
1750
1755
1760
1765
1770
1775
1780
1785
1790
1795
1800
1805
1810
1815
1820
1825
1830
1835
1840
1845
1850
1855
1860
1865
1870
1875
1880
1885
1890
1895
1900
1905
1910
1915
1920
1925
1930
1935
1940
1945
1950
1955
1960
1965
1970
1975
1980
1985
1990
1995
2000
2005
2010
2015
2020
2025
2030
2035
2040
2045
2050
2055
2060
2065
2070
2075
2080
2085
2090
2095
2100
2105
2110
2115
2120
2125
2130
2135
2140
2145
2150
2155
2160
2165
2170
2175
2180
2185
2190
2195
2200
2205
2210
2215
2220
2225
2230
2235
2240
2245
2250
2255
2260
2265
2270
2275
2280
2285
2290
2295
2300
2305
2310
2315
2320
2325
2330
2335
2340
2345
2350
2355
2360
2365
2370
2375
2380
2385
2390
2395
2400
2405
2410
2415
2420
2425
2430
2435
2440
2445
2450
2455
2460
2465
2470
2475
2480
2485
2490
2495
2500
2505
2510
2515
2520
2525
2530
2535
2540
2545
2550
2555
2560
2565
2570
2575
2580
2585
2590
2595
2600
2605
2610
2615
2620
2625
2630
2635
2640
2645
2650
2655
2660
2665
2670
2675
2680
2685
2690
2695
2700
2705
2710
2715
2720
2725
2730
2735
2740
2745
2750
2755
2760
2765
2770
2775
2780
2785
2790
2795
2800
2805
2810
2815
2820
2825
2830
2835
2840
2845
2850
2855
2860
2865
2870
2875
2880
2885
2890
2895
2900
2905
2910
2915
2920
2925
2930
2935
2940
2945
2950
2955
2960
2965
2970
2975
2980
2985
2990
2995
3000
3005
3010
3015
3020
3025
3030
3035
3040
3045
3050
3055
3060
3065
3070
3075
3080
3085
3090
3095
3100
3105
3110
3115
3120
3125
3130
3135
3140
3145
3150
3155
3160
3165
3170
3175
3180
3185
3190
3195
3200
3205
3210
3215
3220
3225
3230
3235
3240
3245
3250
3255
3260
3265
3270
3275
3280
3285
3290
3295
3300
3305
3310
3315
3320
3325
3330
3335
3340
3345
3350
3355
3360
3365
3370
3375
3380
3385
3390
3395
3400
3405
3410
3415
3420
3425
3430
3435
3440
3445
3450
3455
3460
3465
3470
3475
3480
3485
3490
3495
3500
3505
3510
3515
3520
3525
3530
3535
3540
3545
3550
3555
3560
3565
3570
3575
3580
3585
3590
3595
3600
3605
3610
3615
3620
3625
3630
3635
3640
3645
3650
3655
3660
3665
3670
3675
3680
3685
3690
3695
3700
3705
3710
3715
3720
3725
3730
3735
3740
3745
3750
3755
3760
3765
3770
3775
3780
3785
3790
3795
3800
3805
3810
3815
3820
3825
3830
3835
3840
3845
3850
3855
3860
3865
3870
3875
3880
3885
3890
3895
3900
3905
3910
3915
3920
3925
3930
3935
3940
3945
3950
3955
3960
3965
3970
3975
3980
3985
3990
3995
4000
4005
4010
4015
4020
4025
4030
4035
4040
4045
4050
4055
4060
4065
4070
4075
4080
4085
4090
4095
4100
4105
4110
4115
4120
4125
4130
4135
4140
4145
4150
4155
4160
4165
4170
4175
4180
4185
4190
4195
4200
4205
4210
4215
4220
4225
4230
4235
4240
4245
4250
4255
4260
4265
4270
4275
4280
4285
4290
4295
4300
4305
4310
4315
4320
4325
4330
4335
4340
4345
4350
4355
4360
4365
4370
4375
4380
4385
4390
4395
4400
4405
4410
4415
4420
4425
4430
4435
4440
4445
4450
4455
4460
4465
4470
4475
4480
4485
4490
4495
4500
4505
4510
4515
4520
4525
4530
4535
4540
4545
4550
4555
4560
4565
4570
4575
4580
4585
4590
4595
4600
4605
4610
4615
4620
4625
4630
4635
4640
4645
4650
4655
4660
4665
4670
4675
4680
4685
4690
4695
4700
4705
4710
4715
4720
4725
4730
4735
4740
4745
4750
4755
4760
4765
4770
4775
4780
4785
4790
4795
4800
4805
4810
4815
4820
4825
4830
4835
4840
4845
4850
4855
4860
4865
4870
4875
4880
4885
4890
4895
4900
4905
4910
4915
4920
4925
4930
4935
4940
4945
4950
4955
4960
4965
4970
4975
4980
4985
4990
4995
5000
5005
5010
5015
5020
5025
5030
5035
5040
5045
5050
5055
5060
5065
5070
5075
5080
5085
5090
5095
5100
5105
5110
5115
5120
5125
5130
5135
5140
5145
5150
5155
5160
5165
5170
5175
5180
5185
5190
5195
5200
5205
5210
5215
5220
5225
5230
5235
5240
5245
5250
5255
5260
5265
5270
5275
5280
5285
5290
5295
5300
5305
5310
5315
5320
5325
5330
5335
5340
5345
5350
5355
5360
5365
5370
5375
5380
5385
5390
5395
5400
5405
5410
5415
5420
5425
5430
5435
5440
5445
5450
5455
5460
5465
5470
5475
5480
5485
5490
5495
5500
5505
5510
5515
5520
5525
5530
5535
5540
5545
5550
5555
5560
5565
5570
5575
5580
5585
5590
5595
5600
5605
5610
5615
5620
5625
5630
5635
5640
5645
5650
5655
5660
5665
5670
5675
5680
5685
5690
5695
5700
5705
5710
5715
5720
5725
5730
5735
5740
5745
5750
5755
5760
5765
5770
5775
5780
5785
5790
5795
5800
5805
5810
5815
5820
5825
5830
5835
5840
5845
5850
5855
5860
5865
5870
5875
5880
5885
5890
5895
5900
5905
5910
5915
5920
5925
5930
5935
5940
5945
5950
5955
5960
5965
5970
5975
5980
5985
5990
5995
6000
6005
6010
6015
6020
6025
6030
6035
6040
6045
6050
6055
6060
6065
6070
6075
6080
6085
6090
6095
6100
6105
6110
6115
6120
6125
6130
6135
6140
6145
6150
6155
6160
6165
6170
6175
6180
6185
6190
6195
6200
6205
6210
6215
6220
6225
6230
6235
6240
6245
6250
6255
6260
6265
6270
6275
6280
6285
6290
6295
6300
6305
6310
6315
6320
6325
6330
6335
6340
6345
6350
6355
6360
6365
6370
6375
6380
6385
6390
6395
6400
6405
6410
6415
6420
6425
6430
6435
6440
6445
6450
6455
6460
6465
6470
6475
6480
6485
6490
6495
6500
6505
6510
6515
6520
6525
6530
6535
6540
6545
6550
6555
6560
6565
6570
6575
6580
6585
6590
6595
6600
6605
6610
6615
6620
6625
6630
6635
6640
6645
6650
6655
6660
6665
6670
6675
6680
6685
6690
6695
6700
6705
6710
6715
6720
6725
6730
6735
6740
6745
6750
6755
6760
6765
6770
6775
6780
6785
6790
6795
6800
6805
6810
6815
6820
6825
6830
6835
6840
6845
6850
6855
6860
6865
6870
6875
6880
6885
6890
6895
6900
6905
6910
6915
6920
6925
6930
6935
6940
6945
6950
6955
6960
6965
6970
6975
6980
6985
6990
6995
7000
7005
7010
7015
7020
7025
7030
7035
7040
7045
7050
7055
7060
7065
7070
7075
7080
7085
7090
7095
7100
7105
7110
7115
7120
7125
7130
7135
7140
7145
7150
7155
7160
7165
7170
7175
7180
7185
7190
7195
7200
7205
7210
7215
7220
7225
7230
7235
7240
7245
7250
7255
7260
7265
7270
7275
7280
7285
7290
7295
7300
7305
7310
7315
7320
7325
7330
7335
7340
7345
7350
7355
7360
7365
7370
7375
7380
7385
7390
7395
7400
7405
7410
7415
7420
7425
7430
7435
7440
7445
7450
7455
7460
7465
7470
7475
7480
7485
7490
7495
7500
7505
7510
7515
7520
7525
7530
7535
7540
7545
7550
7555
7560
7565
7570
7575
7580
7585
7590
7595
7600
7605
7610
7615
7620
7625
7630
7635
7640
7645
7650
7655
7660
7665
7670
7675
7680
7685
7690
7695
7700
7705
7710
7715
7720
7725
7730
7735
7740
7745
7750
7755
7760
7765
7770
7775
7780
7785
7790
7795
7800
7805
7810
7815
7820
7825
7830
7835
7840
7845
7850
7855
7860
7865
7870
7875
7880
7885
7890
7895
7900
7905
7910
7915
7920
7925
7930
7935
7940
7945
7950
7955
7960
7965
7970
7975
7980
7985
7990
7995
8000
8005
8010
8015
8020
8025
8030
8035
8040
8045
8050
8055
8060
8065
8070
8075
8080
8085
8090
8095
8100
8105
8110
8115
8120
8125
8130
8135
8140
8145
8150
8155
8160
8165
8170
8175
8180
8185
8190
8195
8200
8205
8210
8215
8220
8225
8230
8235
8240
8245
8250
8255
8260
8265
8270
8275
8280
8285
8290
8295
8300
8305
8310
8315
8320
8325
8330
8335
8340
8345
8350
8355
8360
8365
8370
8375
8380
8385
8390
8395
8400
8405
8410
8415
8420
8425
8430
8435
8440
8445
8450
8455
8460
8465
8470
8475
8480
8485
8490
8495
8500
8505
8510
8515
8520
8525
8530
8535
8540
8545
8550
8555
8560
8565
8570
8575
8580
8585
8590
8595
8600
8605
8610
8615
8620
8625
8630
8635
8640
8645
8650
8655
8660
8665
8670
8675
8680
8685
8690
8695
8700
8705
8710
8715
8720
8725
8730
8735
8740
8745
8750
8755
8760
8765
8770
8775
8780
8785
8790
8795
8800
8805
8810
8815
8820
8825
8830
8835
8840
8845
8850
8855
8860
8865
8870
8875
8880
8885
8890
8895
8900
8905
8910
8915
8920
8925
8930
8935
8940
8945
8950
8955
8960
8965
8970
8975
8980
8985
8990
8995
9000
9005
9010
9015
9020
9025
9030
9035
9040
9045
9050
9055
9060
9065
9070
9075
9080
9085
9090
9095
9100
9105
9110
9115
9120
9125
9130
9135
9140
9145
9150
9155
9160
9165
9170
9175
9180
9185
9190
9195
9200
9205
9210
9215
9220
9225
9230
9235
9240
9245
9250
9255
9260
9265
9270
9275
9280
9285
9290
9295
9300
9305
9310
9315
9320
9325
9330
9335
9340
9345
9350
9355
9360
9365
9370
9375
9380
9385
9390
9395
9400
9405
9410
9415
9420
9425
9430
9435
9440
9445
9450
9455
9460
9465
9470
9475
9480
9485
9490
9495
9500
9505
9510
9515
9520
9525
9530
9535
9540
9545
9550
9555
9560
9565
9570
9575
9580
9585
9590
9595
9600
9605
9610
9615
9620
9625
9630
9635
9640
9645
9650
9655
9660
9665
9670
9675
9680
9685
9690
9695
9700
9705
9710
9715
9720
9725
9730
9735
9740
9745
9750
9755
9760
9765
9770
9775
9780
9785
9790
9795
9800
9805
9810
9815
9820
9825
9830
9835
9840
9845
9850
9855
9860
9865
9870
9875
9880
9885
9890
9895
9900
9905
9910
9915
9920
9925
9930

means. The electronic circuitry is externally powered or it may contain an internal power source.

The capsule advances through the GI tract due to the normal intestinal action (contraction and relaxation of the GI tract muscular tissue). Due to its
5 small size the capsule leaves the body with the excrement anally.

In a preferred embodiment of the present invention the housing of the capsule is made of dissolvable material (such as the material used for producing medication capsules), so that in the event of pathological narrowing of the intestines the capsule will not be stuck there. Naturally such material
10 should be made durable enough so that it may pass the entire GI tract without disintegrating during the estimated period of time it would normally take for the capsule to pass through.

As it may be possible for the capsule to roll over and turn around when it advances through the GI tract the capsule is provided with dual optics so
15 that in fact it includes two viewing means oppositely directed. This feature is also important when the view of the front viewing optics is locally obstructed by a protrusion on the surface rising from the intestine wall (like a polyp).

The system is supplemented by external receiving unit for receiving the data transmitted from the capsule, and a control unit for processing said data
20 and displaying the images obtained.

Figure 1b illustrates a general view of an encapsulated medical imaging device in accordance with a preferred embodiment of the present invention. The capsule 1, in this example having a housing 40 of elongated dimensions, comprises two optical setups, each having an axial hemispherical
25 symmetry and located at either ends of the capsule. The capsule housing 40 is provided with arms 42 having flat feet 4 substantially covering cavities 44 in which the foldable arms are housed (see also Figures 2a and 2b and the corresponding description in this specification for the use and operation of these arms). Each end of the capsule is provided with a front lens 2, for

viewing objects in front of that end, light emitting diodes (LED) 3 for illuminating a sector in close proximity of the capsule (at least covering the whole range of the optical focused field of view of the optical components of the device), and an array of microlenses 9 made up of a multiple rows of microlenses (depicted in these Figures, for the sake of simplicity, are only four
5 rows 5, 6, 7, and 8, but in reality a much larger number of rows of microlenses is employed). The optical set-up is described in detail with reference to Figures 3a, 3b, 4a and 4b). For example, microlens arrays are commercially available from MEMS Optical Inc (Huntsville, Alabama, USA).

10 The LED diodes 3 may optionally be sources of light in different frequencies, for example omitting light in the RGB ranges (i.e. one omitting red, another omitting green and yet another omitting blue light). This is to allow scanning in different monochromatic illumination by turning on separately and sequentially each LED color and then combining the different
15 mono-chromatic gray-scale images into one color image by the processing means of the system.

An optional wiper 97 is provided comprising a wiping arm traveling over the microlens array, bound by tracks 99, so as to cover the entire microlens array, and wipe dirt off the lenses.

20 Further optional feature is a sensor 98 for sensing medical parameters such as local temperature, pressure or other parameters that communicates with the electronic control of the capsule and thus capable of transmitting the sensed data to an external receiver.

Figure 2a illustrates the encapsulated medical imaging device of the
25 present invention provided with arms, shown in semi-retracted state as it travels through a small intestine. The arms 42 of the device are provided so as to provide support for the device against the intestine wall 34 as the arms' feet 4 lean against the wall, and prevent the device from flopping over or turning sideways. The arms may be resilient or mechanically foldable and
30 deployable so as to apply slight counter-force onto the intestine wall and

enhance its supporting ability. The arms may alternatively or complementarily be sampling means, for sampling tissue or matter from the intestine wall. In the latter case, the arms are each adapted to be operated separately (via controlling means) and adapted to be able to be retracted into its corresponding cavity 44 so as to keep the sample inside the cavity once it is retrieved.

Figure 2b depicts the encapsulated medical imaging device of Fig. 2a with its support arms deployed as it travels through a large intestine. As the large intestine 36 is wider the arms may employ fully and reach to the intestine wall so as to prevent disorientation of the capsule.

In another preferred embodiment of the present invention, feet 4 may be as large as the entire housing, or substantial portions of it, thus providing larger contact surface with the intestinal wall.

Figure 3a is a see-through view of a preferred embodiment of the encapsulated medical imaging device of the present invention. Microlens array 9 focuses light reflected from image outside the capsule. It is noted that each microlens may see different view, as some face certain sector and others face other sectors. An optical array is provided inside the capsule, typically comprising an array of light-sensitive receiving cells 12. As the embodiment shown in the figures has twin optical set-up, aimed at providing two counter-directional viewing ability, two optical arrays are provided, positioned back to back so that each faces one end of the device, located in the focal plane of the corresponding optical set-up. The complete image imprinted on the optical array is a result of aggregation of images obtained by each microlens. The optical array is sampled for data by corresponding electronic circuitry 11, which samples in a predetermined manner rows or columns or any other predetermined arrangement, and convert the analog data to digital data. The device is in fact scanning the image in scanning technology.

Optionally it may be required to place appropriate correction optical lenses 52, 54 between each optical array and its corresponding optical set-up. Electronic control units 10, 11 are each electrically communicating with the optical arrays, as well as controlling the light diodes 3, and powering them.

5 The control unit is adapted to generate transmission of data obtained by the optical array to an external receiver.

It is possible to provide the device with internal power source, such as a battery, or provide inductive circuitry (see for example US 4,278,077 to Mitsumoto) that is powered by induction from an external inductive source.

10 Figure 3b depicts the optical scheme of the device of Fig. 3a. Each microlens of microlens array 9 views a small sector of the hemispherical surroundings of the device, and is focused via the optical lenses to an appropriate corresponding cell of the optical array. Front and back images are focused through the front and back lenses 2 onto central area 78 of the optical array, whereas the peripheral image obtained by coronal microlens array 9 is
15 focused onto an outer annular strip portion 76. Identically, the image obtained by the optics of the other end of the capsule is focused on central area 74 and peripheral area 72 of the optical array.

It is stipulated that if the curvature of the microlens array 9 corresponds
20 to the curvature of the front lens 2, than a continuous image of the objects viewed outside the capsule may be obtained. Alternatively two separate images may be displayed on an external monitor – one of the view from the front lens and one of the peripheral view viewed by the microlens array. A combined image may also be constructed. In a preferred embodiment of the
25 present invention, all image manipulation is carried out by an external processing unit (as described hereafter).

Figure 4a illustrates a single stretched row of the microlens array of the device of Fig. 3a. In a preferred embodiment of the present invention the microlens array comprises a plurality of microlenses 22, arranged in a
30 sequential manner with lenses having different focal distance distributed in

that row. The different foci lenses are arranged so that for a particular angle of view there exist all types of the various microlens lens, and each lens is focused on a corresponding cell of the light receiving array of cells (such as photoelectric cells). A first group of lenses is focused on an imaginary plane
5 60 located at a first predetermined distance from the array. A second group of lenses is focused on an imaginary plane 62 located at a second predetermined distance from the array, closer than plane 60. A third group of lenses is focused on an imaginary plane 64 located at a third predetermined distance from the array closer still. This way the microlens array has three
10 focus planes and not only one.

The virtue of this feature can be appreciated by referring to Figure 4b, illustrating fields of view of an encapsulated medical imaging device in accordance to the present invention as it travels through an intestine.

As the capsule arrives (position 1a) some portions of the intestine walls
15 39 are hidden as a protrusion 37 blocks its field of view. In fact the inside walls of the intestine are very irregular. Chyme (mixed food and digestive juices) is pushed through the small intestine through muscular contractions. During these contractions the chyme, having the consistency of runny applesauce, is squished into the lining of the wall of the small intestine. Nutrients are
20 absorbed via osmosis by the blood vessels in the mesentery and absorbed through osmosis by the blood vessels attached to the outside of the small intestine. The lining of the intestine is hilly so as to present large surface area for that osmosis to take place. However when the capsule crosses over to position 1b its rear optics allows viewing that hidden area and thus the
25 limitations of the prior art devices concerning their field of view is greatly reduced.

It is clearly seen that the capsule may be positioned in different distances 31, 33, 29, 51) from the intestine wall lining. If an inspected object is located at a certain distance 31 that equals to the focal distance of one of the
30 microlens groups, than its best available image will be acquired from that lens

(in fact from a plurality of close lenses from that same group). The control unit of the device or the external monitoring means which receive the transmission is preferably provided with image processing software adapted to identify only focused images and disregard blurred images obtained from the other lens groups. Thus the device is capable of providing clear and focused images of objects at various distances from the device. The processing unit is thus adapted to identify and distinguish focused image data from unfocused one, disregard the unfocused data and acquire image made of focused data only.

Similarly, in another preferred embodiment of the present invention, an alternative optical setup may include multiple multi-focal lenses.

Figures 5a, 5b and 5c illustrate a display monitor communicating with a receiving unit of an encapsulated medical imaging device of the present invention incorporated in a vest 21 worn by a patient. Vest 21 houses the receiving unit adapted to communicate with the capsule and may also include powering means such as inductive circuitry. It engulfs the patients' torso effectively close to the capsule as it travels through the patient's GI tract. The receiving unit in the vest communicates via cable or wirelessly with monitoring unit 139. Monitoring unit 139 provided with display means for displaying one or several images 17, 18, by the encapsulated medical imaging device and/or other data 16.

Figure 6 illustrates the path traveled by a capsule in a patient's small intestine. In another preferred embodiment of the present invention the device incorporates with monitoring means adapted to identify the position and location within the GI tract where an image was acquired by comparing it to a prearranged library of images, and identifying by image processing the type of environment the capsule was in when the image was acquired. It is stipulated that each portion of the GI track (i.e. esophagus, small intestine, large intestine stomach) has unique image (texture, shape, and other distinct features). By identifying the type of environment the device was in when the image was acquired and by knowing some parameters such as the sampling

rate of the device, its traveling velocity within the GI tract (on average it is assumed that it would travel at the rate of 1 to 3 cm per second) it is possible to determine or at least estimate the distance of the path 94 traveled by the capsule from the last identified position 92 to the current location 96, where a pathology was detected and viewed by the capsule. The software may generate a general view of the GI tract, the last image obtained as the device entered into the current type of GI tract and most recent image obtained. A graphic indication on the general image, in the form of a cursor, arrow or any other graphical representation, may be superposed on the GI tract image indicating the device current (or recent) location. This can substantially enhance the medical team's ability to locate the exact position of the pathology found in position 96.

Figure 7 illustrates an optional schematic configuration of the electronic system of an encapsulated medical imaging device in accordance with a preferred embodiment of the present invention. This is given as an example only. A person skilled in the art could easily provide other electrical configurations that would still be covered by the scope of the present invention.

The capsule 100 generally comprises optics 110 (the lens es and optical array) communicating with a control unit 112 that transmits the digital data obtained from the optical array via communication interface 114 and antenna 116. The capsule is optionally inductively powered by an inductive circuitry 111 energized externally by inductance. A receiver 102 (such as one incorporated in a vest – see Figures 5b and 5c) picks up the data transmitted by an antenna 118 and communicates with a control unit 104. The control unit comprises communication interface 120, control unit 122, processor 124, and display means 126 (such as a monitor). It is optionally also provided with a user interface 128, for inputting commands to the control unit. In a preferred embodiment of the present invention the control unit is programmed or programmable so that physician can adjust the sampling rate of the device (i.e. the frequency of image acquiring), control the foldable arms, choose the

images to be displayed or command the system to perform calculations (such as the distance traveled by the capsule inside the intestine).

5 The advantages of the encapsulated imaging device of the present invention are numerous. The device provides high accessibility to the entire GI tract. The unique optical setup provides better images and a greater range for focused images. Optional sampling arms may be operated in-vivo and obtain samples such as biopsy, blood test or retrieve any other sample from the matter the device comes near to. External energizing prevents the need for internal power source that may be hazardous to the patient if the capsule
10 disintegrates within the GI tract.

In a preferred embodiment of the present invention the images may be obtained by scanning in RGB light – first scanning in red light, then scanning in green and finally in blue, each time obtaining mono-chromatic gray-scale quality images and incorporating them into a color image by the processing
15 means of the external unit and presenting the color image on the monitor.

Note that the system described in the specification and figures is mainly designed to obtain black and white images, but these images are remarkably clear and distinct and the anticipated resolution is much greater than that of video images.

20 It should be clear that the description of the embodiments and attached Figures set forth in this specification serves only for a better understanding of the invention, without limiting its scope as covered by the following Claims.

It should also be clear that a person skilled in the art, after reading the present specification could make adjustments or amendments to the attached
25 Figures and above described embodiments that would still be covered by the following Claims.

C L A I M S

1. An encapsulated medical imaging system comprising:

a capsule of swallowable proportion comprising:

5 at least one optical setup of a number of optical setups comprising an array of microlenses distributed in axial symmetry on at least a portion of the capsule so that the array of microlenses is capable of receiving light reflected from object located in at least a sector outside the capsule;

10 corresponding optical array comprising an array of light sensitive cells optically communicating with said optical setup through focusing means, such that the image of the object is focused on the array of light sensitive cells;

15 electronic circuitry adapted to sample image data obtained by the optical array by scanning the image and converting the image data to digital data;

illuminating means for illuminating a sector in front the optical setup, outside the capsule;

20 transmitting means communicating with said electronic circuitry, adapted to receive image digital data and transmit it to an external receiver;

receiving means for receiving data transmitted from said capsule;

image processing means for processing the data received by the receiving means and; and

display means for displaying an image.

25

2. The system as claimed in Claim 1, wherein the number of the optical setups comprises two optical setups, arranged in opposite sides of the capsule, so as to allow counter-directional viewing.
3. The system as claimed in Claim 1, wherein it is provided with at least one lens of a number of lenses for central view and wherein the array of
5 microlenses is arranged in a coronal arrangement with respect to the lens, so as to provide peripheral view.
4. The system as claimed in Claim 3, wherein the number of lenses comprises two lenses.
- 10 5. The system as claimed in Claim 1 wherein the microlens array comprises a plurality of microlenses having different foci distributed in a known distribution, and wherein the processing means is adapted to identify and distinguish focused image data from unfocused one, disregard the unfocused data and acquire image made of focused data only.
- 15 6. The system as claimed in Claim 1, wherein the illumination means comprises light emitting diodes.
7. The system as claimed in Claim 6, wherein the light emitting diodes illuminate light in different frequency ranges.
8. The system as claimed in Claim 7, wherein the light emitting diodes
20 emit red, green or blue light.
9. The system as claimed in claim 8, wherein the light emitting diodes are operated so as to sequentially illuminate red green and blue light.
10. The system as claimed in Claim 1, wherein the capsule is about 12-20 mm in length and about 5-7 mm in diameter.
- 25 11. The system as claimed in claim 1, wherein the capsule housing is made from a biocompatible material.

12. The system as claimed in Claim 1, wherein the capsule housing is made from a dissolvable material.

13. The system as claimed in Claim 12, wherein the capsule housing is made from a dissolvable material that is durable enough so that it may pass
5 an entire GI tract without disintegrating during the estimated period of time it would normally take for the capsule to pass through.

14. The system as claimed in Claim 1, wherein the capsule is internally powered.

15. The system as claimed in Claim 1, wherein the capsule is externally
10 powered.

16. The system as claimed in Claim 15, wherein the capsule is inductively powered.

17. The system as claimed in Claim 16, wherein the capsule is further provided with supporting means for supporting the capsule and preventing its
15 turning over or around.

18. The system as claimed in Claim 17, wherein said supporting means comprise extractable surfaces.

19. The system as claimed in Claim 17, wherein the extractable surfaces are supported by arms.

20. 20. The system as claimed in Claim 19, wherein said arms are resilient.

21. The system as claimed in Claim 19, wherein said arms are mechanically foldable.

22. The system as claimed in Claim 19, wherein the arms are adapted to be housed in cavities provided in the housing of the capsule.

25 23. The system as claimed in Claim 22, wherein the cavities are adapted to hold samples obtained by the arms.

24. The system as claimed in Claim 1, wherein the capsule is further provided with a medical parameter sensor.

25. The system as claimed in Claim 24, wherein the sensor comprises a temperature sensor or a pressure sensor.

5 26. The system as claimed in Claim 1, wherein the capsule is further provided with wiping means for wiping dirt off the optical setup.

27. The system as claimed in Claim 26, wherein the wiping means comprises a wiping arm.

28. An encapsulated medical imaging system comprising:

10 a capsule of swallowable proportion comprising:

at least one optical setup of a number of optical setups comprising an array of multi-focal lenses distributed in axial symmetry on at least a portion of the capsule so that the array of multi-focal lenses is capable of receiving light reflected from object located in at least a sector outside the capsule;

15

corresponding optical array comprising an array of light sensitive cells optically communicating with said optical setup through focusing means, such that the image of the object is focused on the array of light sensitive cells;

20 electronic circuitry adapted to sample image data obtained by the optical array by scanning the image and converting the image data to digital data;

illuminating means for illuminating a sector in front the optical setup, outside the capsule;

transmitting means communicating with said electronic circuitry, adapted to receive image digital data and transmit it to an external receiver;

receiving means for receiving data transmitted from said capsule;

5 image processing means for processing the data received by the receiving means and; and

display means for displaying an image.


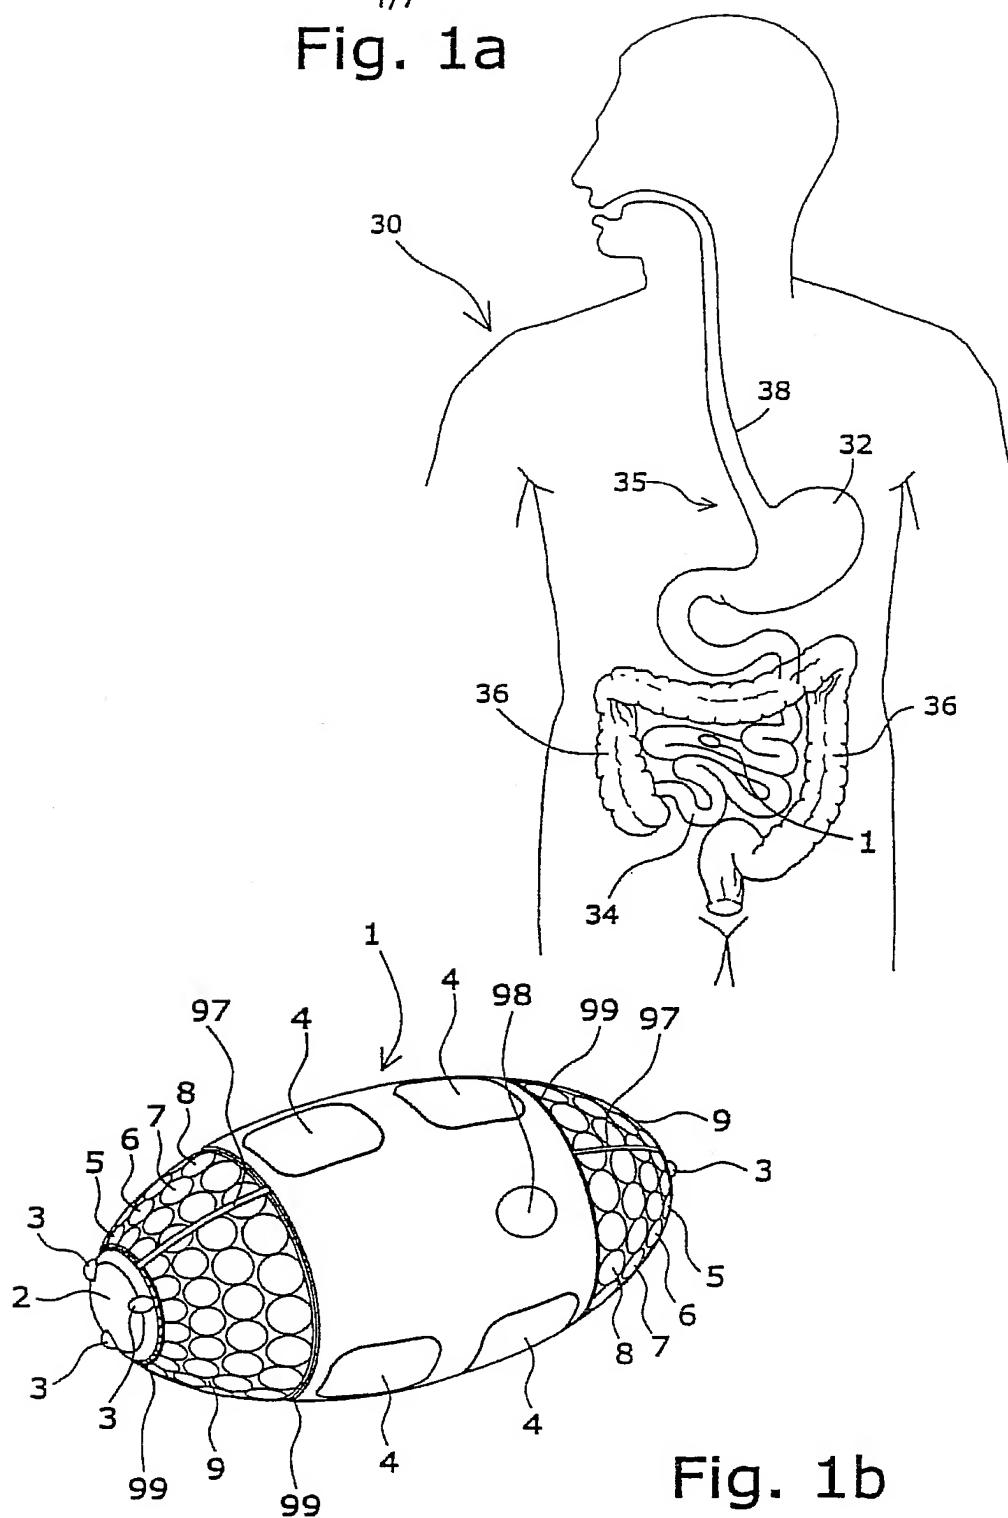
1/7
Fig. 1a

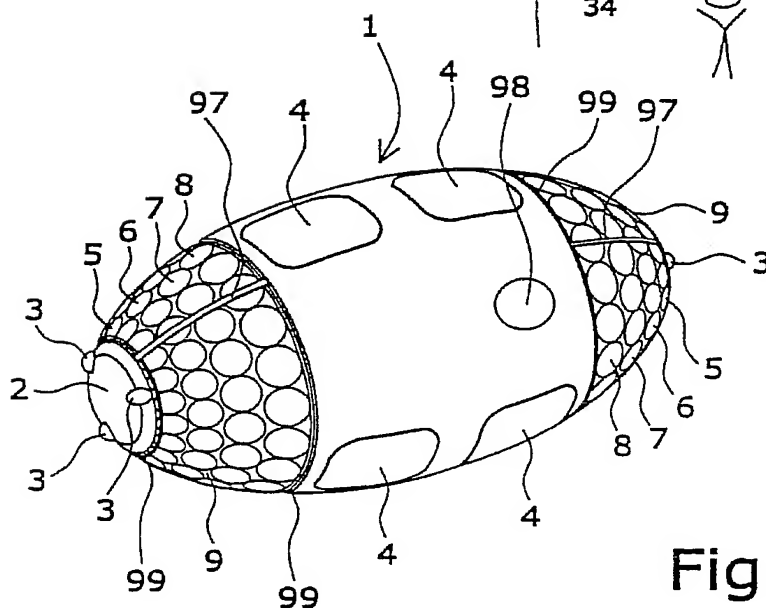Fig. 1b



2/7

Fig. 2a

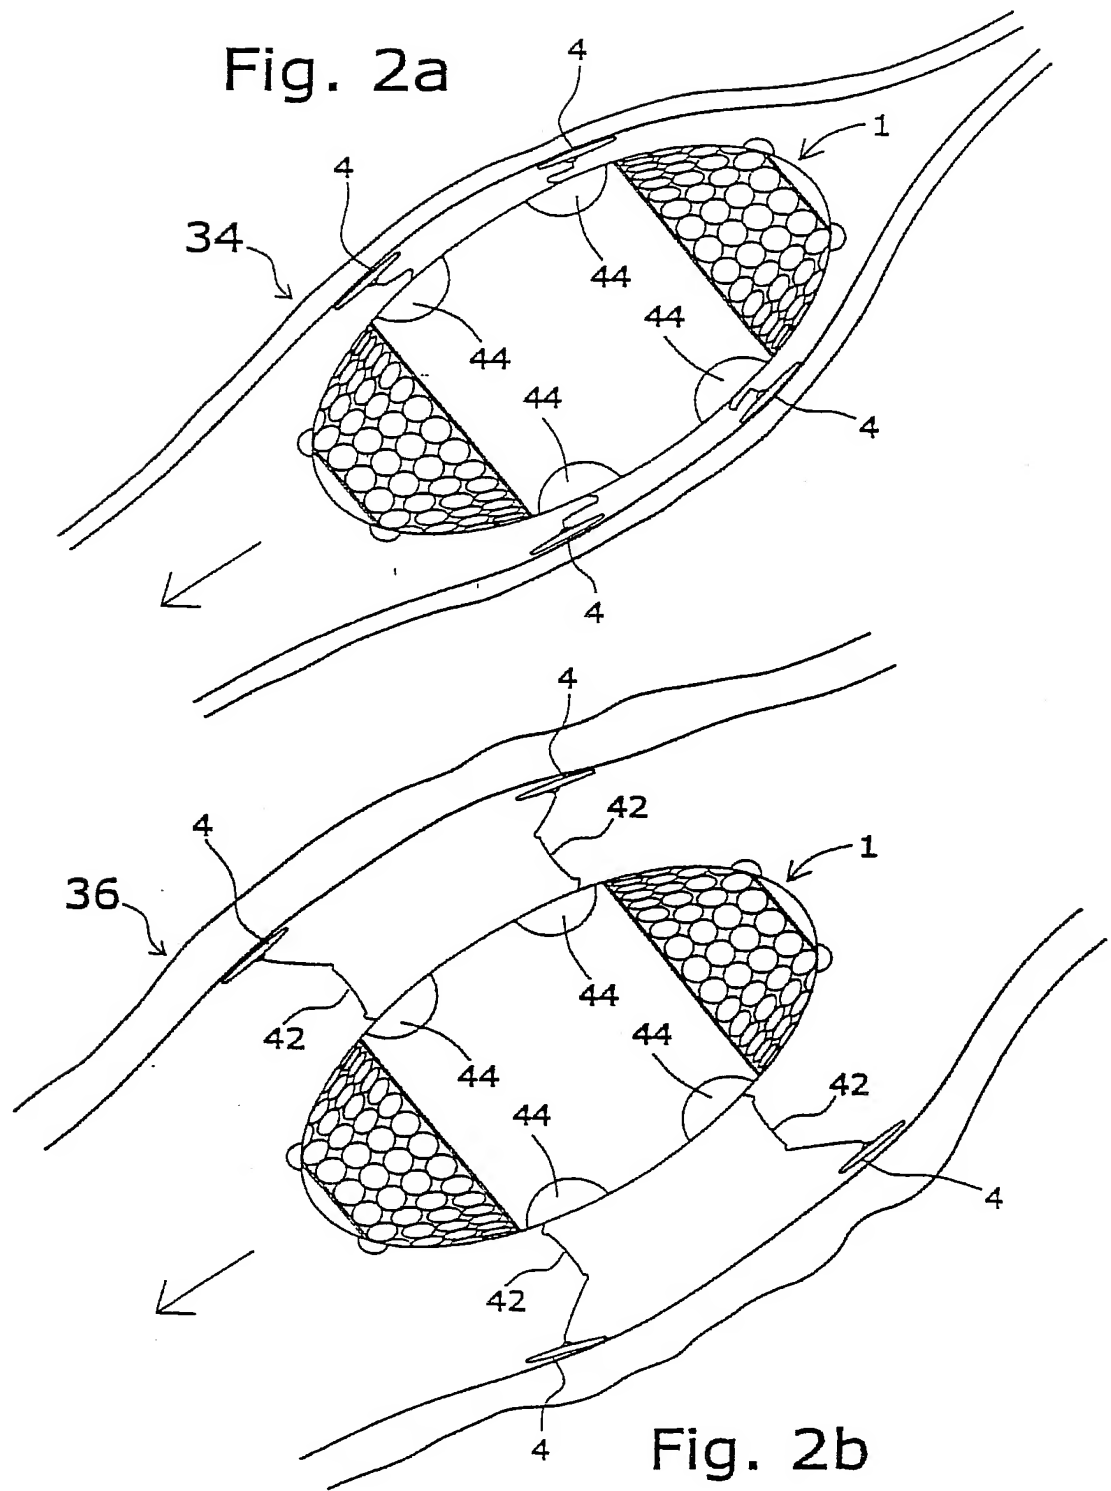


Fig. 2b

Fig. 3a

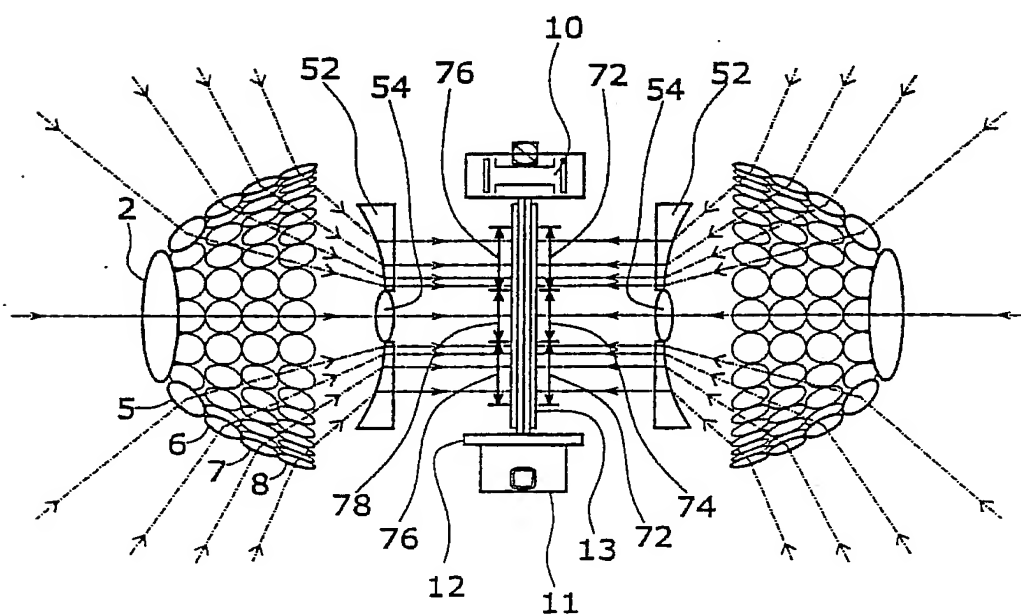
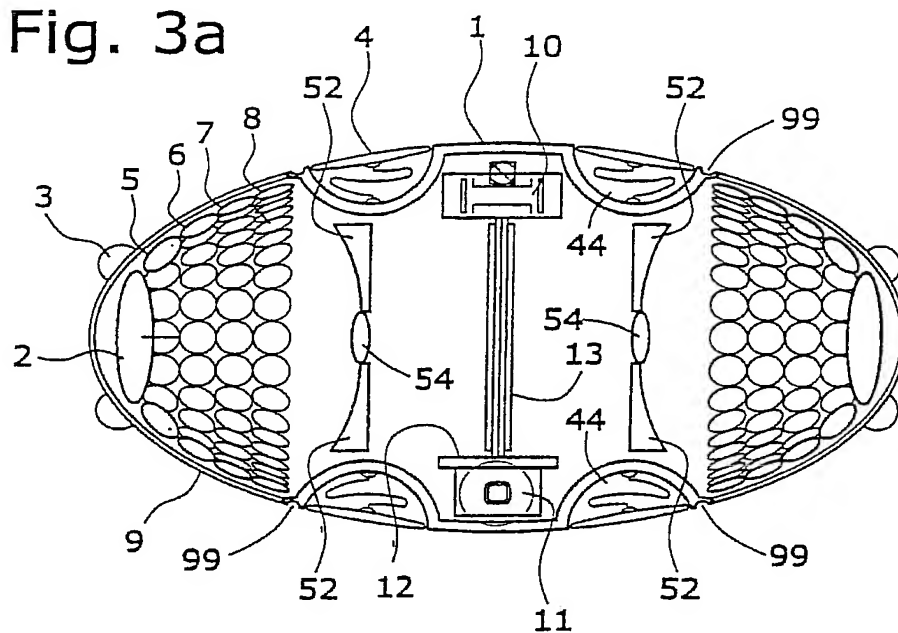


Fig. 3b

4/7

Fig. 4a

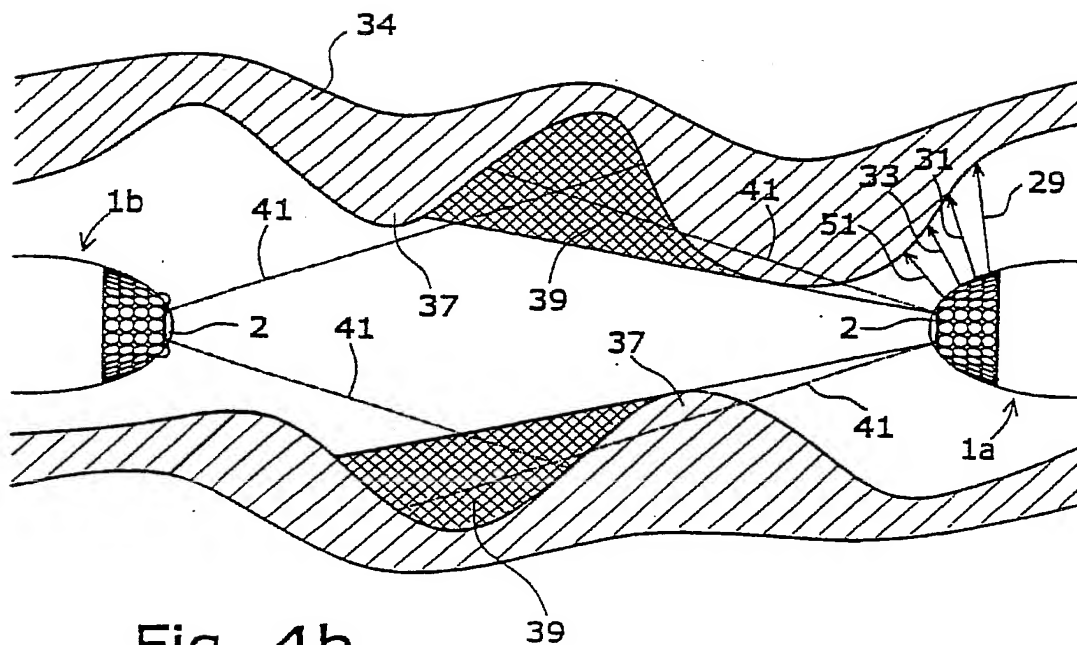
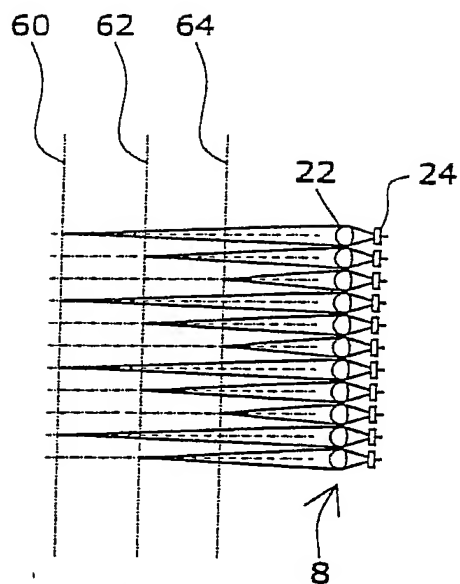


Fig. 4b

Fig. 5a

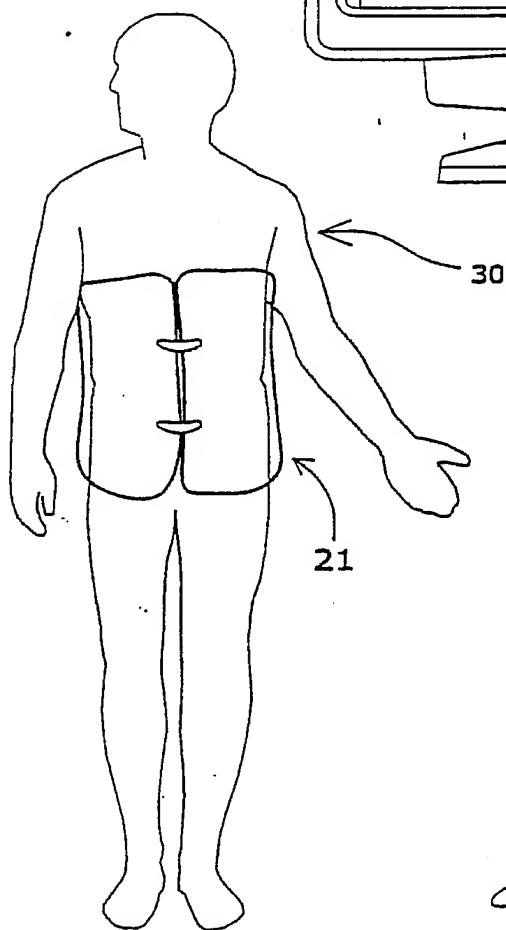
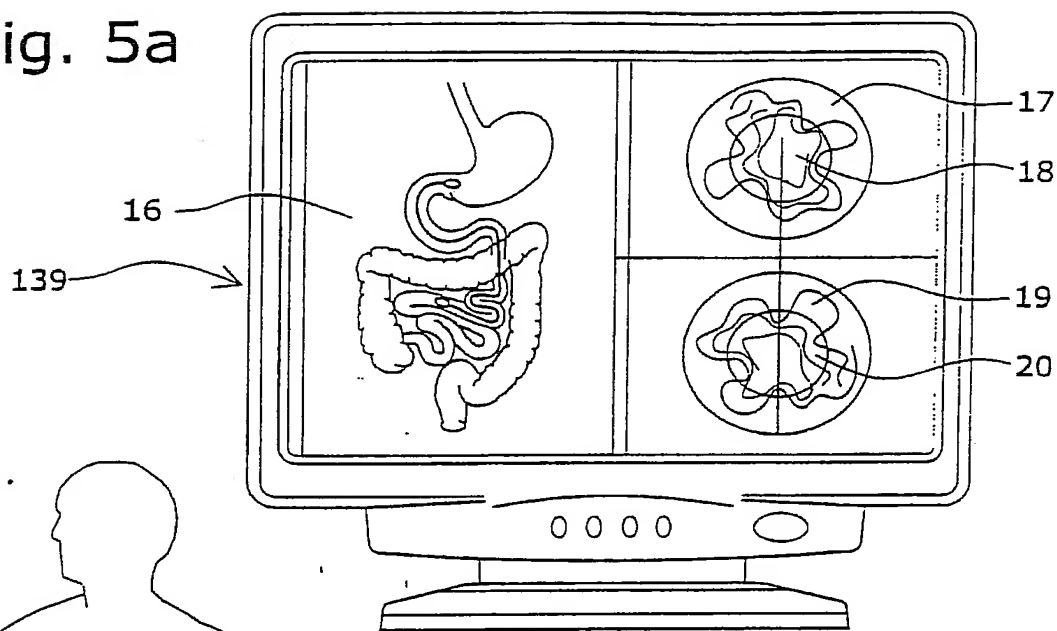


Fig. 5b


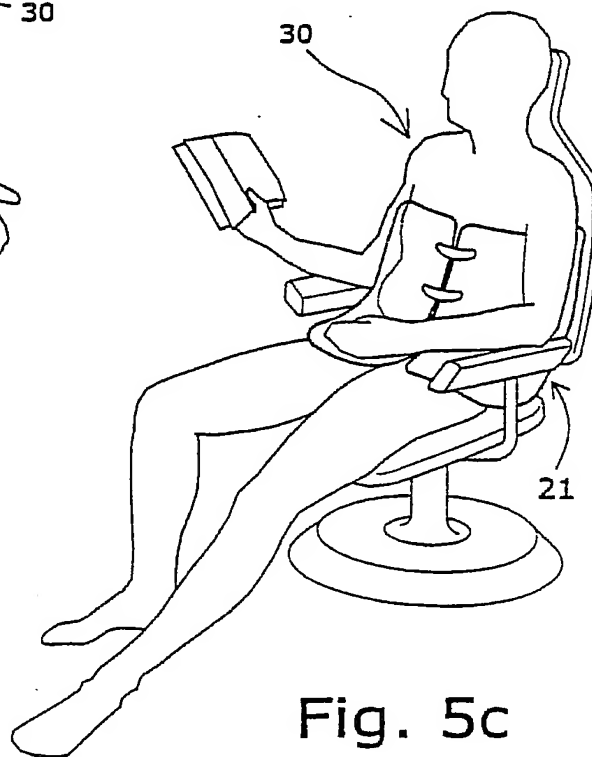


Fig. 5c

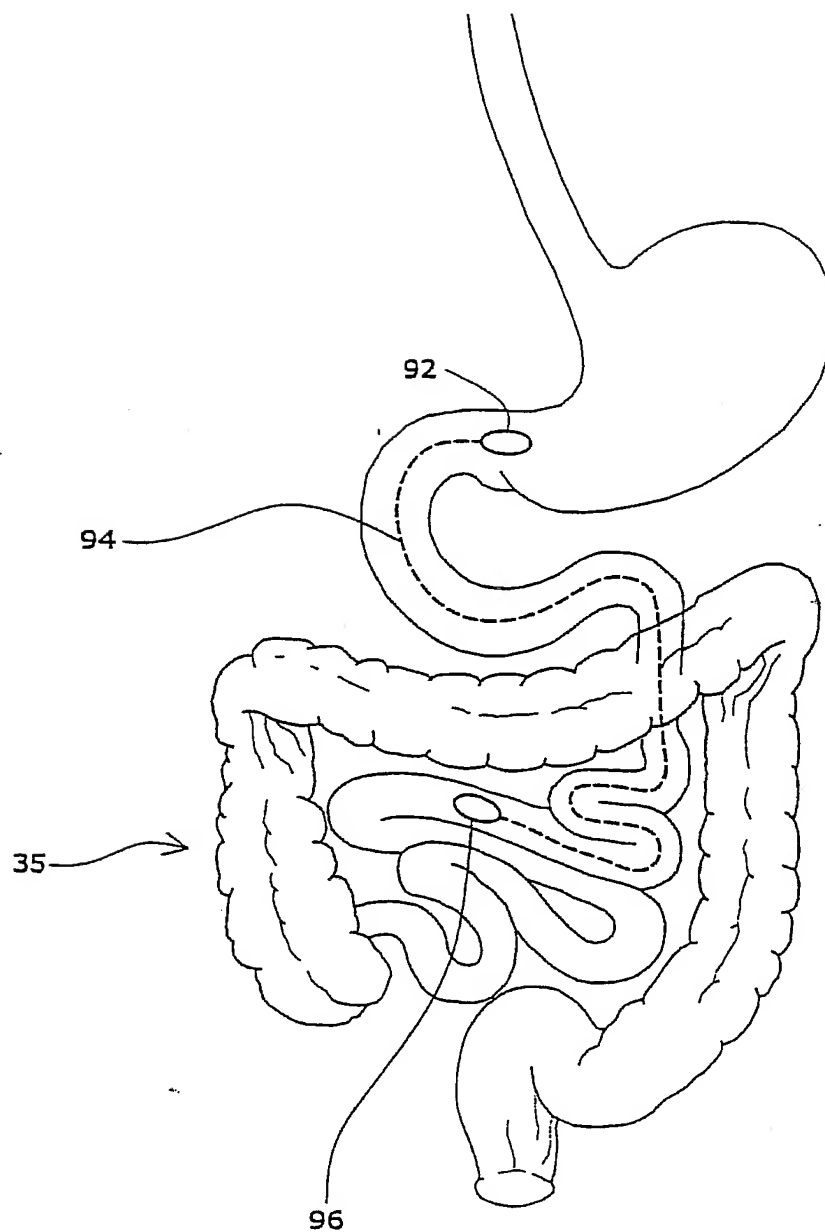Fig. 6



7/7

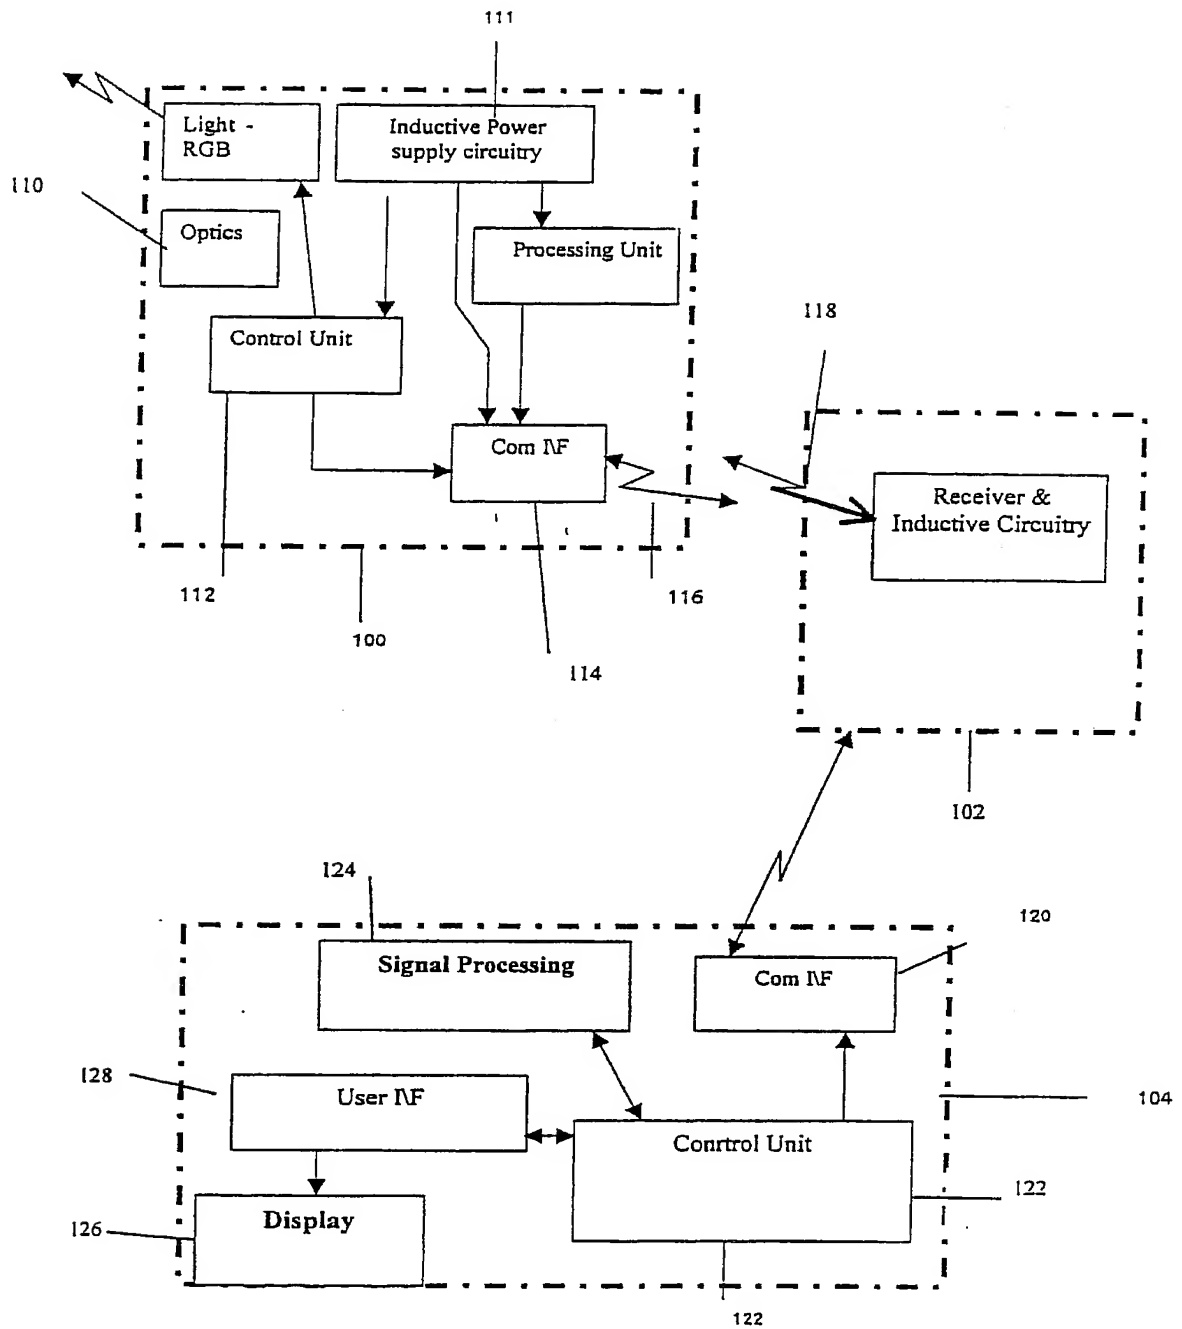


FIG 7